


**Challenging Conventional Boundaries**



*Fit n Feel*<sup>™</sup>

**Powder - Free HIGH PERFORMANCE  
Nitrile Examination Gloves**

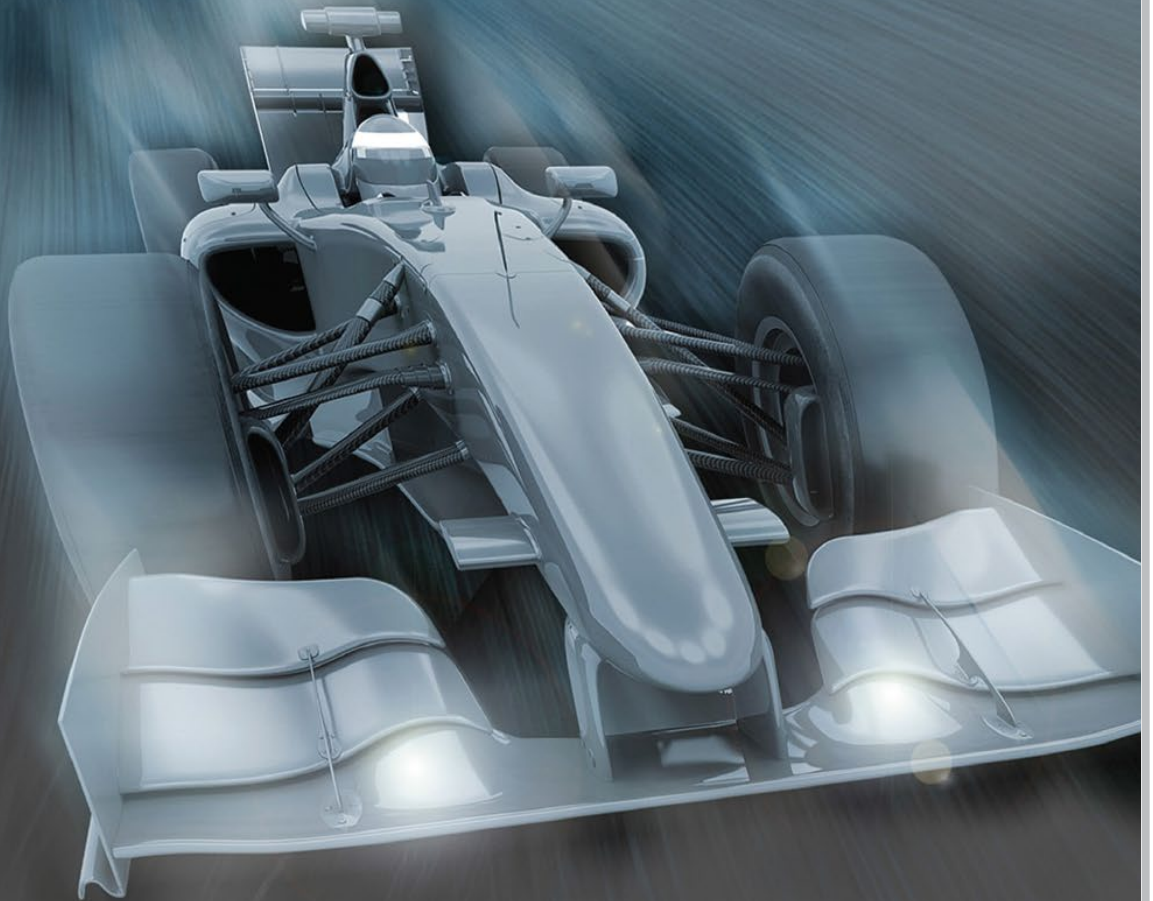

# Fit To Applications, Feel The Performance And Precision

## Glove Design

Ambidextrous • Finger Textured • Beaded Cuff • 9" Cuff Length • Powder-free • Available in Blue & White Color • Freedom from Hole : G1 / AQL 1.5

## Technical Product Information

Parameter	Typical Performance*
<b>Dimension</b>	
Finger Thickness (mm)	0.08 - 0.09
Palm Thickness (mm)	0.06 - 0.07
Cuff Thickness (mm)	0.04 - 0.05
Glove Length (mm)	245 ± 0.5
<b>Physical Properties (During Shelf Life)</b>	
Tensile Strength (MPa)	28 - 32
Ultimate Elongation (%)	520 - 560
Force at Break (N)	6.2 - 6.8

\*Typical product performance not to be taken as actual product specification

## Packaging Information

Packaging Style	250pcs / dispenser (2500pcs / carton)	300pcs / dispenser (3000pcs / carton)
<b>20'GP, case</b>	1134 cartons (2.8 Mil. pcs)	945 cartons (2.8 Mil. pcs)
<b>40'GP, case</b>	2250 cartons (5.6 Mil. pcs)	1912 cartons (5.7 Mil. pcs)
<b>40'HC, case</b>	2646 cartons (6.3 Mil. pcs)	2353 cartons (7 Mil. pcs)

## Our Product Testaments



Summarized below is the product performance we have conducted on *Fit n Feel*™ Examination Glove.

Test Parameter	Test Result														
EN 374:2003 part 3: Determination of resistance to permeation by chemicals (EC Certificate, PPE Category III)	<i>Fit n Feel</i> ™ achieved performance Level 6 (>480 minutes breakthrough time) for chemicals as follows: <table border="1" style="margin: 10px auto;"> <tr> <td>50% Sulphuric Acid</td> <td>5% Ethidium Bromide</td> </tr> <tr> <td>10-13% Sodium Hypochlorite</td> <td>50% Glutaraldehyde</td> </tr> <tr> <td>40% Sodium Hydroxide</td> <td>1.5% Methanol in water</td> </tr> <tr> <td>0.1% Phenol</td> <td></td> </tr> </table>	50% Sulphuric Acid	5% Ethidium Bromide	10-13% Sodium Hypochlorite	50% Glutaraldehyde	40% Sodium Hydroxide	1.5% Methanol in water	0.1% Phenol							
50% Sulphuric Acid	5% Ethidium Bromide														
10-13% Sodium Hypochlorite	50% Glutaraldehyde														
40% Sodium Hydroxide	1.5% Methanol in water														
0.1% Phenol															
Food Contact Test (21 CFR 177.2600)	<i>Fit n Feel</i> ™ meet the specification set forth in 21 CFR 177.2600														
Chemotherapy Drugs Permeation Test (ASTM D 6978-05 (2013))	13 out of 15 chemotherapy drugs tested do not breakthrough up to 240 minutes, which are listed as follows : <table border="1" style="margin: 10px auto;"> <tr> <td>Cyclophosphamide (Cytoxan)</td> <td>Methotrexate</td> </tr> <tr> <td>Doxorubicin HCl</td> <td>Mitomycin C</td> </tr> <tr> <td>5 - Fluorouracil</td> <td>Vincristine</td> </tr> <tr> <td>Cisplatin</td> <td>Mitoxantrone</td> </tr> <tr> <td>Etoposide</td> <td>Cytarabine</td> </tr> <tr> <td>Paclitaxel (Taxol)</td> <td>Ifosfamide</td> </tr> <tr> <td>Dacarbazine (DTIC)</td> <td></td> </tr> </table>	Cyclophosphamide (Cytoxan)	Methotrexate	Doxorubicin HCl	Mitomycin C	5 - Fluorouracil	Vincristine	Cisplatin	Mitoxantrone	Etoposide	Cytarabine	Paclitaxel (Taxol)	Ifosfamide	Dacarbazine (DTIC)	
Cyclophosphamide (Cytoxan)	Methotrexate														
Doxorubicin HCl	Mitomycin C														
5 - Fluorouracil	Vincristine														
Cisplatin	Mitoxantrone														
Etoposide	Cytarabine														
Paclitaxel (Taxol)	Ifosfamide														
Dacarbazine (DTIC)															
Skin Irritation & Sensitization Test (ISO 10993-10:2010)	<i>Fit n Feel</i> ™ demonstrates no sensitization & irritation under the test condition induced?														
Viral Penetration Test (ASTM F1671-13)	<i>Fit n Feel</i> ™ pass the test criteria														




## How do we compare with the rest in terms of protection and performance?

Glove Film Strength (the higher the value the stronger is the glove)

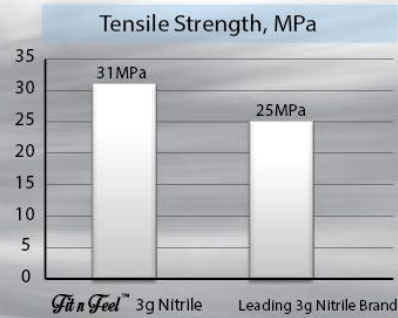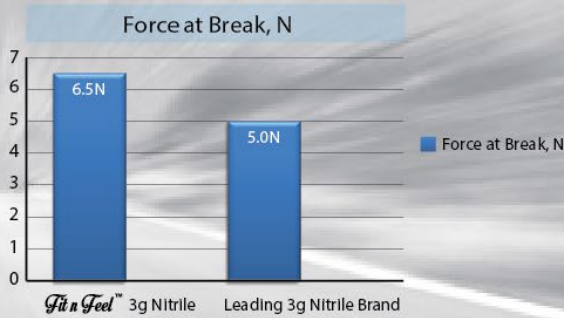

## Glove Chemical & Chemodrug Resistance


Resistance to permeation by chemical (EN 374:2003 Part 3)

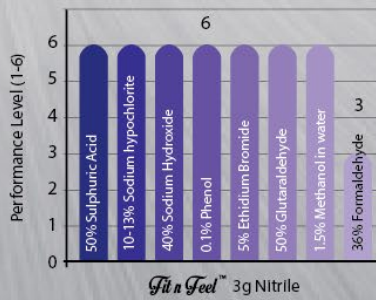

EN 374:2003 part 3: Determination of resistance to permeation by chemical (EC Certificate, PPE Category III)


- Performance Level 3 -> with measured breakthrough time of minimum 60 minutes
- Performance Level 6 -> with measured breakthrough time of minimum 480 minutes

Chemotherapy Drugs Permeation test (ASTM D6978-05 (2013))

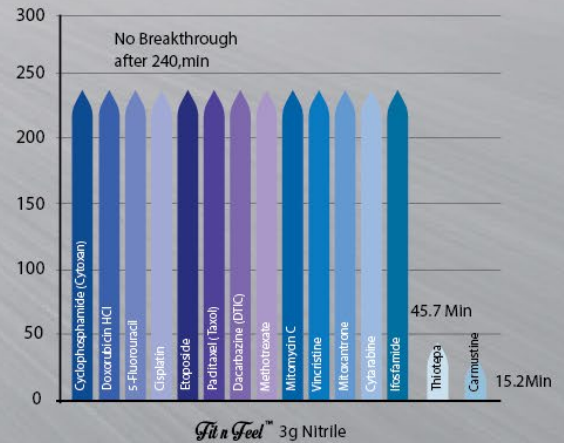

## Supply Chain Savings

With *Fit n Feel*™ optimized packing capabilities; we have studied the estimated savings in the supply chain in comparison with a regular examination glove packing configuration of 100pcs per dispenser pack in a 40' container load.

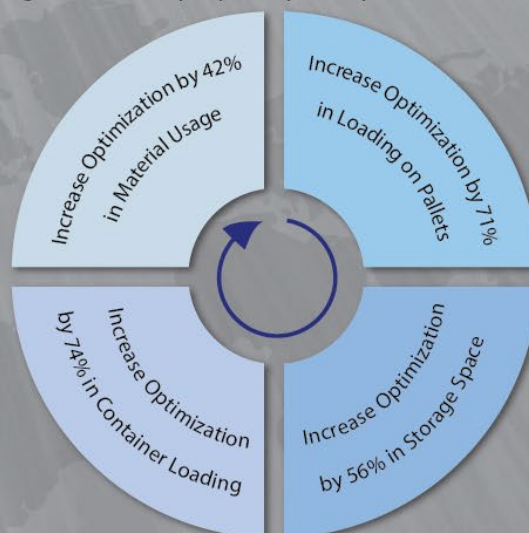

## AN ALL-NEW EXPERIENCE FOR HAND PROTECTION POWERED BY ADVANCE TECHNOLOGY.

- **Ultimate Tactile Sensitivity. *Take control with precision.***

*Fit n Feel™* is designed to provide an incredible feel in tactile sensitivity as if you were not wearing a glove!

- **Excellent Film Strength. *Minimize failures.***

Barrier protection is a crucial aspect for glove protection; *Fit n Feel™* stays true to this by providing high level of protection in film strength, durability and chemical resistance properties.

- **European PPE, Category III Chemical Permeation Tested. *Wide coverage in hand protection.***

*Fit n Feel™*'s strong chemical resistance demonstrates the performance and functionality of the gloves for a wide range of applications. The gloves were designed to enhance user's hand protection.

- **Cleaner Surface. *Ease of use.***

*Fit n Feel™* is innovatively designed with a low friction surface to enhance ease of donning, so users can efficiently glide on *Fit n Feel™* without constraints.





**Medguard Professional Healthcare Supplies**

**Tel: +353 (0) 1 8352411**

**Email: [sales@medguard.ie](mailto:sales@medguard.ie)**

**Fax: +353 (0) 1 969 5009**

**Website: [www.medguard.ie](http://www.medguard.ie)**