

## PRODUCT INFORMATION

**Product Name** BASICBilly+ Upgrade Kit  
**Item No.** 1022626 / P72+AOK  
**Model** AK2G-BI  
**Authorization Code** CE.

### CAUTION

- Keep the used batteries out of reach of children and dispose separately.
- If you do not use BASICBilly+ Upgrade Kit for a long period of time remove and store the batteries.
- Do not use a new battery and an old battery together.



Medguard Professional Healthcare

Tel: +353 (0) 1 835 2411


Email: [sales@medguard.ie](mailto:sales@medguard.ie)

Fax: 01 969 5009

Website: [www.medguard.ie](http://www.medguard.ie)

Unit 6/7, Block 4, Ashbourne Business Park, Ashbourne, Co. Meath, A84 VK52

# BASICBilly+ Upgrade Kit USER GUIDE

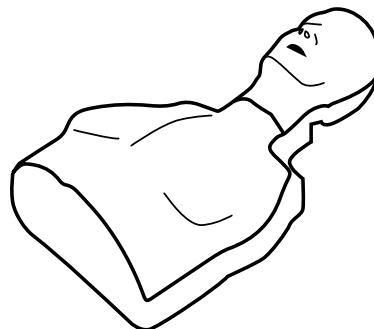

## WARRANTY

1 Manufacturer offers a LIMITED WARRANTY against any defects in workmanship or materials under normal use for one (1) year from the date of purchase. Any component of the BASICBilly+ Upgrade Kit which proves defective within the warranty period will be repaired, free of charge. The customer is responsible for shipping and handling fees to the place which manufacturer designates.



2 Customer must provide proof of the date of purchase, place of purchase and the purchase price in order to obtain service under this limited warranty. No agent, representative, dealer of Manufacturer has the authority to alter the obligations or limitations of this limited warranty.

3 CUSTOMER'S SOLE AND EXCLUSIVE REMEDY AGAINST MANUFACTURE SHALL BE FOR THE REPAIR OR REPLACEMENT OF DEFECTIVE GOODS AS PROVIDED HEREIN. Repair of any component of any BASICBilly+ Upgrade Kit does not extend this limited warranty or begin a new limited warranty period.


4 Manufacturer reserves the right to refuse warranty service or replacement when product failure is due to abrasion, abnormal use, misuse, mishandling, misapplication, accident, neglect, improper installation, modification, use of unauthorized parts or attachments, adjustments or repair performed by anyone other than manufacturer or its authorized agent, or any causes other than defective workmanship or material. This limited warranty does not cover failure or damage resulting from unsuitable operating environments or storing environments or natural disasters or acts of God. MANUFACTURER SHALL NOT BE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES ARISING OUT OF THE USE OF THE BASICBilly+ Upgrade Kit OR THE BREACH OF THIS OR ANY OTHER EXPRESSED OR IMPLIED WARRANTY.



## LIST OF COMPONENTS

- User Guide
- Add-on kit (w/ ventilation sensor)  
Requires 2 "AA" batteries (not included).  
3.0V  $\approx$  100mA (Using two Alkaline 1.5 V Batteries)
- Lung bag with sensor holder
- Color ID Stickers









## DOWNLOAD APPS



- 2)
- 3)  CPR add-on kit Student  
 CPR add-on kit Instructor

# HOW TO INSTALL

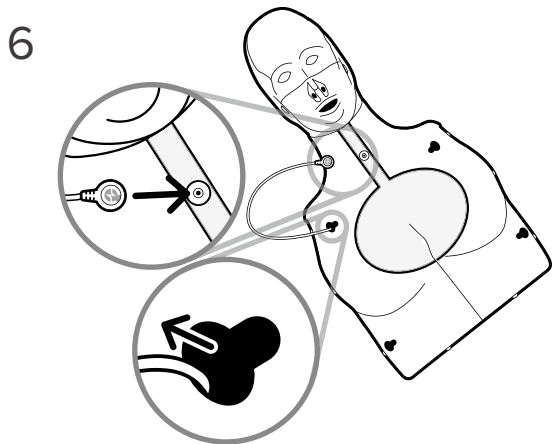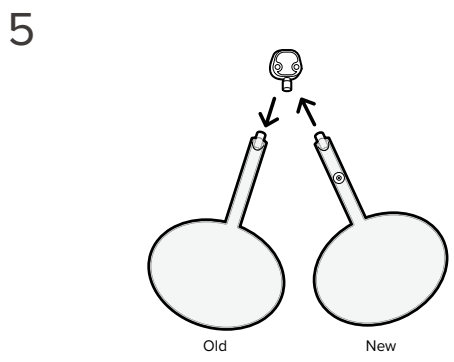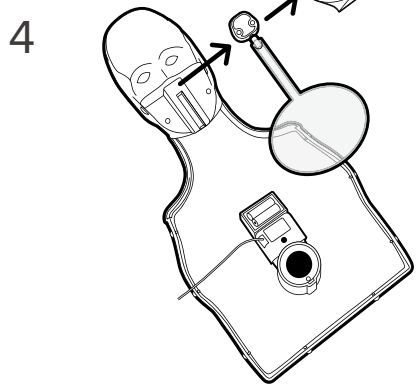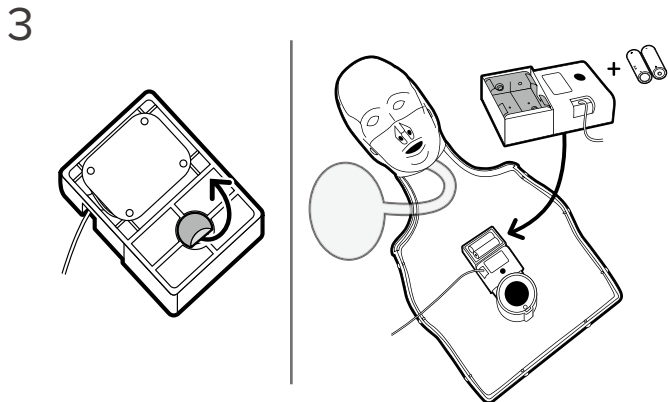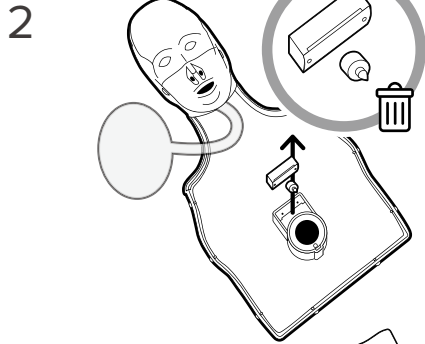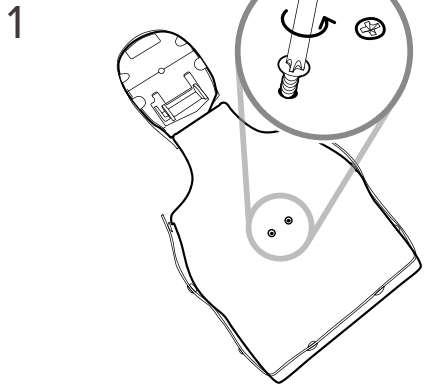

Actual product may vary slightly from photo.  
3B Scientific reserves the right to change product color, materials, supplies, or function as needed.